

This is the peer reviewed version of the following article:

In vivo kinematics of knee replacement during daily living activities: Condylar and post-cam contact assessment by three-dimensional fluoroscopy and finite element analyses / Belvedere, Claudio; Leardini, Alberto; Catani, Fabio; Pianigiani, Silvia; Innocenti, Bernardo. - In: JOURNAL OF ORTHOPAEDIC RESEARCH. - ISSN 0736-0266. - 35:7(2017), pp. 1396-1403. [10.1002/jor.23405]

Terms of use:

The terms and conditions for the reuse of this version of the manuscript are specified in the publishing policy. For all terms of use and more information see the publisher's website.

27/04/2024 10:12

Research Article

**IN-VIVO KINEMATICS OF KNEE REPLACEMENT DURING DAILY LIVING
ACTIVITIES: CONDYLAR AND POST-CAM CONTACT ASSESSMENT BY
THREE-DIMENSIONAL FLUOROSCOPY AND FINITE ELEMENT ANALYSES[†]**

Running title: Contact Assessment in Total Knee Replacement

**Claudio Belvedere¹, Alberto Leardini¹, Fabio Catani², Silvia Pianigiani³, Bernardo
Innocenti⁴**

1. Movement Analysis Laboratory and Functional-Clinical Evaluation of Prostheses, Istituto Ortopedico Rizzoli, Bologna, Italy;
2. Orthopaedics and Traumatology Department, Modena Policlinic, Modena, Italy.
3. Istituto Ortopedico Galeazzi, Milano, Italy
4. BEAMS Department, Université Libre de Bruxelles, Bruxelles, Belgium.

Corresponding Author: Claudio Belvedere, PhD

Movement Analysis Laboratory and Functional-Clinical Evaluation of Prostheses

Istituto Ortopedico Rizzoli

Via di Barbiano 1/10, 40136 – Bologna, Italy

Tel: +39 051 6366570 / Fax: +39 051 6366561 / Email: belvedere@ior.it

Author Contributions Statement: Each author has been involved either in the study design, or in the performance of the analysis, or in data interpretation, or in the manuscript drafting. All authors have read and approved the final submitted manuscript.

[†]This article has been accepted for publication and undergone full peer review but has not been through the copyediting, typesetting, pagination and proofreading process, which may lead to differences between this version and the Version of Record. Please cite this article as doi: [10.1002/jor.23405]

Received 29 June 2016; Revised 1 August 2016; Accepted 26 August 2016

Journal of Orthopaedic Research

This article is protected by copyright. All rights reserved

DOI 10.1002/jor.23405

ABSTRACT

In total knee replacement, the investigation on the exact contact patterns at the post-cam in implanted patients from real in-vivo data during daily living activities is fundamental for validating implant design concepts and assessing relevant performances. This study is aimed at verifying the restoration of natural tibio-femoral condylar kinematics by investigating the post-cam engagement at different motor tasks. An innovative validated technique, combining three-dimensional fluoroscopic and finite element analyses, was applied to measure joint kinematics during daily living activities in 15 patients implanted with guided motion posterior-stabilized total knee replacement. Motion results showed physiological antero-posterior translations of the tibio-femoral condyles for every motor task. However, high variability was observed in the position of the calculated pivot point among different patients and different motor tasks, as well as in the range of post-cam engagement. Physiological tibio-femoral joint rotations and contacts at the condyles were found restored in the present knee replacement. Articular contact patterns experienced at the post-cam were found compatible with this original prosthesis design. The present study reports replaced knee kinematics also in terms of articular surface contacts, both at the condyles and, for the first time, at the post-cam.

This article is protected by copyright. All rights reserved

Keywords: total knee replacement, tibio-femoral kinematics, three-dimensional video-fluoroscopy, condylar contacts, post-cam contact, daily living activities, finite element analysis.

This article is protected by copyright. All rights reserved

INTRODUCTION

Posterior-Stabilized total knee replacement has been introduced in the mid-1970s¹ as an alternative to cruciate retaining designs. The reasons for this innovation are: firstly, to cater for clinical cases of missing or dysfunctional posterior-cruciate ligament (PCL) and, secondly, to achieve a more natural knee kinematics^{1,2}. The posterior-stabilized design, particularly for its post-cam mechanism feature, was also meant to avoid posterior subluxation of the tibia, in a way to substitute the degenerated PCL, and to improve the range of knee flexion by allowing femoral roll-back, which potentially can also increase the quadriceps moment arm³⁻⁵. This design is also expected to limit excessive antero-posterior tibial translation, after resection of the PCL. Posterior-Stabilized total knee replacement has been widely used for more than two decades for patients requiring primary or revision knee replacement, and long-term follow-up studies have reported satisfactory results^{2,6-8}. Intra- and post-operative benefits of a posterior stabilized over a cruciate retaining knee replacement, include easier ligament balancing and easier correction of possible severe deformities (by eliminating tight PCL), better restoration of knee kinematics, increased stability and range of motion, reduced quadriceps force in extension and potentially minimized polyethylene wear when more congruent articular surfaces are used⁹⁻¹¹. However, complications and potential disadvantages include fracture and wear of the tibial post, soft-tissue impingement, and risks of dislocation or instability during flexion¹²⁻¹⁷.

In-vivo kinematics of replaced knees during weight and non-weight bearing activities, by using three-dimensional (3D) fluoroscopy, has been largely reported^{7,8,18-24}. These studies demonstrated high variability among patients, among surgeons and also among different implant designs. Patterns of the so-called paradoxical kinematics, i.e. anterior translation of the femur during knee flexion, have also been shown. Such paradoxical motion results in reduced knee flexion and effective muscle lever arm of both agonist and antagonist muscle

groups^{19,25,26}. Antero-posterior translation and axial rotation at the tibio-femoral prosthetic articulation during weight bearing activities is highly dependent on the geometry of the tibial insert. Most of the knee prostheses have been designed to have a distinguished antero-posterior contact between femur and tibial insert. Tibio-femoral contact points should be at about 2/3 of the antero-posterior length of the tibial insert, in order to increase knee flexion and to optimize the extensor mechanism. In this way a good restoration of the PCL function is obtained by the post-cam^{24,25,27-29}. The former mechanism, also obtained by the symmetrical and concave geometry of the polyethylene insert at the medial and lateral condyles, is likely to be the main reason for the physiological internal rotation of the tibia during knee flexion, as shown in a number of fluoroscopy data^{18-21,30}.

The paradoxical joint motion observed in replaced knees pertains not only the anterior translation of the femur during flexion, but also its posterior translation during extension^{19,20,31}, both likely associated to the post-cam design^{3,24,32-35}. Therefore, using computer-based kinematic modeling^{36,37}, this mechanism has been modified to more constraining contacts, particularly at the anterior aspect of the post-cam^{7,21,33,38}, designed to mimic the physiological motion of the knee joint. In particular, with this more recent design, the anatomical dishing of the insert, i.e. concave geometry in the medial side and convex geometry in the lateral side, and the asymmetric post-cam mechanism, with different anterior and posterior aspects of the cam were meant to result in the physiological roll-back of the femur during flexion.

The amount of antero-posterior translation at the tibio-femoral joint, and of post-cam engagement during stair, step up, lunge and squatting exercises has been investigated; the related results showed a nearly physiological knee kinematics^{7,8,39,40}. However, fluoroscopy-based assessments have mainly focused on tibio-femoral translation and axial rotation, and only a few papers have investigated the full post-cam mechanism during weight and non-weight bearing activities. More specifically, detailed assessments of the exact contact patterns

at the post-cam in implanted patients from real in-vivo data during daily living activities are expected to provide fundamental information for validating implant design concepts and assessing relevant performances, but these are not yet available in the literature.

In this study, an innovative validated technique, combining 3D fluoroscopic and finite element analyses³³, was applied to analyze a group of 15 patients who underwent total knee replacement with a constraining post-cam design, during several daily living activities. The aims of our study were 1) to verify whether a constrained post-cam mechanism resulted in physiological knee joint kinematics; 2) to analyze the knee flexion range at which the post-cam mechanism engages; and 3) to investigate the influence of different motor tasks on the post-cam mechanism and on the position and translation of the tibio-femoral contact points.

MATERIALS AND METHODS

Fifteen patients (Table 1) affected by primary knee osteoarthritis were implanted with a post-cam fixed-bearing prosthesis (Journey[®] Bi-Cruciate Stabilized Knee System; Smith & Nephew, Inc, Memphis, TN-USA). This design claims a better restoration of natural knee kinematics by means of a larger constraining effect, implied by the new post-cam mechanism and by the original shapes of the medial and lateral condyles^{7,41,42}. At 6 months after surgery, all patients were evaluated clinically and by 3D video-fluoroscopy in order to derive joint motion at the replaced knee. This is an analytical and retrospective study (Level of Evidence III), conducted after institutional review board approval and in conformity with local ethical regulations; written informed consent was obtained from all patients prior surgery.

In the post-operative clinical evaluation at follow-up, all patients showed good outcome according to the International Knee Society scoring system⁴³ (corresponding “knee” and “function” mean scores being about 94.9 and 90.7, respectively; the thorough clinical assessment of the present cohort can be found in⁷). As for 3D kinematic evaluation, a

fluoroscopic device (digital remote-controlled diagnostic Alpha90SX16; CAT Medical System, Rome, Italy) was used for image acquisitions in a 32-cm-wide field of view during cycles of chair rising-sitting, stair climbing, and step up-down at 10 Hz sampling frequency^{7,8,39}. The height of the staircase steps was 21 cm.; the chair height was set for each patient to allow about 80° of initial knee flexion when sitting^{7,8,39}. The 3D position and orientation of the femoral and tibial prosthesis components were derived from fluoroscopic images after a preliminary image calibration phase and by an iterative procedure using a shape-matching technique based on the CAD models of the implanted prosthesis (tested translational/rotational accuracy: 0.5 mm / 1.0°)⁴⁴. Corresponding knee joint kinematics was derived using a standard joint convention⁴⁵, resulting in relatively normal knee kinematics associated to roll-back and screw-home mechanisms⁷.

Using a previously validated numerical technique³³, in-vivo 3D kinematics obtained from video-fluoroscopy was used as input for a patient specific finite element model of the implant; this was then used to calculate, for each patient and for each motor task, the contact between the femoral and tibial components, therefore both at the condyles and at the post-cam. For the latter, three possible situations were considered: anterior contact, posterior contact, and no contact between cam and post. The femoral component was considered a rigid body and was represented by triangular surfaces (about 11,500 elements); the tibial insert was represented by eight-node 3D hexahedrals (about 15,500 elements). The tibial insert was considered as the fixed reference, and the femoral component was considered to move according to the aforementioned in-vivo joint kinematics. Material models, properties and friction coefficient were chosen according to the literature^{33,46,47}. All simulations were performed using Abaqus/Explicit version 6.10-1 (Dassault Systèmes, Vélizy-Villacoublay, France). For each patient and motor task, the 3D coordinates of the medial and lateral femoral condylar contact points on the tibial insert and the tibio-femoral axial rotation, as assessed via finite element

analysis, were plotted versus the knee flexion angle. In detail, the contact points were determined by the software as the centroid of the pressure distribution of the medial and lateral femoral condyles on the tibial insert during motion; the contact-line was defined as the line connecting the medial and lateral contact points. The position of the corresponding pivot point was estimated as the least-square approximation of the intersection of all the contact lines calculated throughout the joint motion. This was reported as percentage locations over the antero-posterior length of the tibial insert for normalization, with -50% and 50% being respectively the most posterior and most anterior location. It was also normalized over the medio-lateral width of the tibial insert, -50% and 50% being respectively the most lateral and most medial location. Both length and width of the tibial insert were extracted from relevant computer-aided-drafting models. Furthermore, knee flexion angles at the point of contact of the post-cam, were also determined.

RESULTS

Consistent patterns over patients and motor tasks were observed for the antero-posterior displacement of the medial and lateral condylar contact points versus knee flexion (Figure 1).

The range of this antero-posterior displacement at the lateral condyle (about 26, 18 and 30 mm in chair rising, stair climbing and step-up, respectively) is almost double than the one observed at the medial condyle (12, 10 and 15 mm, respectively). This implies an overall internal rotation of the tibia during flexion and also a good restoration of the natural roll-back and screw-home mechanisms at the replaced knee.

Consistent patterns among patients were also observed for the axial rotation of the femoral component with respect to the tibial component (Figure 2). In particular, the knee rotates internally during knee flexion, from about 8° external rotation to about 8° internal rotation. Specifically, the ranges from full extension to maximum flexion were different among the

different motor tasks, these being 10.3°, 14.8°, and 20.4° in chair rising, stair climbing and step-up, respectively. When the analysis of this range is limited to the first 30° flexion, the rotation is limited to 6.6°, 5.6° and 10.1°, respectively.

The normalized position of the pivot point was found in a postero-medial location (chair rising, stair climbing and step-up tasks shown in Figure 3, 4 and 5, respectively), although the results show also high variability among patients and motor tasks, particularly in the medio-lateral direction.

This can be appreciated also by looking at these positions when superimposed from all patients and motor tasks (Figure 6), and at the range of rotation of the contact line and the location of the pivot point for each patient and for each motor task for the full range of flexion (Table 2).

As for post-cam contact mechanism, the analysis of the engagement of the tibial post revealed that the contacts of its anterior and posterior parts with the femur cam occur more frequently at small and larger flexion angles, respectively. Particularly, the anterior contact (Figure 7a) started at maximum extension, i.e. mostly in hyper-extension, in all motor tasks and continued till about 10° flexion. At 0° flexion, anterior contact is experienced, according to the motor task, in 40% to 60% of the observed knees. As for the engagement at the posterior aspect of the post (Figure 7b), a much higher variability was found, both among patients and motor tasks. Particularly, contact can occur before 20° flexion in some cases, while at 30° in others; about 60-70% of patients revealed posterior post-cam engagement at 80° flexion.

DISCUSSION

In general, the present study was aimed at assessing, with a robust technique, joint motion in the replaced knee, but, particularly and originally, it was aimed at substantiating the post-cam engagement both in its anterior and posterior aspects. To this purpose, a recently published validated technique³³, which combines in-vivo 3D fluoroscopic kinematics and finite element

analysis, was applied on joint motion data from a cohort of patients during three standard activities of daily living. The results of the present analyses provided enough evidence for the three aforementioned aims. In particular, aim 1), physiological patterns and ranges of motion were consistently observed at the replaced knees among patients; these were also found to be consistent with the preliminary results of the present cohort and technique ³³, as well as with previous fluoroscopic studies ^{20,21,48}. The post-cam mechanism, aim 2), specifically at the anterior and posterior aspect of the post, occurred respectively during knee extension, particularly toward hyperextension, and from 80° flexion onward, though a high variability among patients was observed between 20° and 80° flexion. Interestingly, about 15% of patients did not show any post-cam engagement. This post-cam engagement varied considerably over the analyzed motor tasks, aim 3), apart from the effect on the antero-posterior translation of the tibio-femoral contact points, which was similar among the three different motor tasks.

A number of in-vivo studies have reported high variability in kinematic patterns at the replaced knee, as associated to different prostheses, even within the posterior-stabilized design. Paradoxical tibio-femoral motion has also been shown in the presence of post-cam ^{3,19,20,31,32,34,35}. However, there was a lack of knowledge on the influence of the post-cam mechanism on the amount of antero-posterior translation of the two contact points, on the medial and lateral tibial condyles. In the present study, the consistent posterior translation of the femur contact on the lateral tibial condyle is remarkably larger than the one on the medial tibial condyle, very similarly to what occurs in the natural knee ⁴⁹. The restoration of the physiological screw home mechanism is revealed here in the analyzed knees, independently from the motor task, by the posterior contact translations and large axial rotation combined to flexion. This likely results from the present design of the prosthesis that features a double shaped post-cam and a dishing geometry at the tibial condyles in the rest of the polyethylene

insert, which should also provide intrinsic joint stability. A large internal rotation was observed throughout the knee range from hyperextension to the maximum flexion, apart from the range between 10° and 35°. This is very important, particularly considering that the restoration of the normal axial rotation is essential also to gain physiological flexion in weight bearing⁵⁰. As for the post-cam mechanism and its engagements, the observed high variability over patients and over motor tasks may be accounted for to the subject-specific action of the agonist and antagonist muscles, necessary for knee balancing during highly demanding weight bearing activities. For example, an early post-cam engagement, together with a more posterior position of the lateral condyle contacts, occurred at the beginning of stair climbing, i.e. at the extension phase, at about 80° flexion associated with the initial monopodal lifting of the body (Fig.7b). The effect of the post-cam mechanism, combined with the magnitude and pattern of axial rotation in these replaced knees, was also a general medial location for the pivot contacts point. This effect was observed in all three motor tasks, though the pivot point position was slightly more lateral in the step-up than in the other two tasks (Fig. 3). This concurs with the literature, where the pivot point position was shown to depend upon the prosthesis design and the locomotor tasks^{8,18,39,48}. However, an overall variability, in terms of knees motion patterns and pivot and contact point positions, has been observed also in normal, i.e. physiological, knees⁴⁹.

The present study is limited by the number of patients analyzed, but the overall consistency of the results support the value of the study. It is confirmed that the finite element analysis performed on the results of the 3D video-fluoroscopy analysis contributes to a smoother and coherent final joint motion, particularly important for sensitive kinematics analyses such as the calculation of pivot point locations.

In conclusion, the present study reports kinematics of the femoral and tibial components in replaced knees, not only in terms of standard joint motion along the three anatomical planes,

but also in terms of articular surface contacts, both at the condyles and, for the first time, at the post-cam. Specifically, physiological tibio-femoral joint rotations and contacts at the condyles were found restored in the present knee replacement. Articular contact patterns experienced at the post-cam were found compatible with this original prosthesis design.

ACKNOWLEDGMENTS

This work was supported by the Italian Ministry of Economy and Finance, programme “5 per mille.”

REFERENCES

1. Insall JN, Hood RW, Flawn LB, Sullivan DJ. 1983. The total condylar knee prosthesis in gonarthrosis. A five to nine-year follow-up of the first one hundred consecutive replacements. *J. Bone Joint Surg. Am.* 65:619-628.
2. Nakayama K, Matsuda S, Miura H, Iwamoto Y, Higaki H, Otsuka K. 2005. Contact stress at the post-cam mechanism in posterior-stabilised total knee arthroplasty. *J. Bone Joint Surg. Br.* 87:483-488.
3. Li G, Most E, Otterberg E, Sabbag K, Zayontz S, Johnson T, Rubash H. 2002. Biomechanics of posterior-substituting total knee arthroplasty: an in vitro study. *Clin. Orthop. Relat Res.*404:214-225.
4. Most E, Zayontz S, Li G, Otterberg E, Sabbag K, Rubash HE. 2003. Femoral rollback after cruciate-retaining and stabilizing total knee arthroplasty. *Clin. Orthop. Relat Res.*410:101-113.
5. Stern SH, Insall JN. 1992. Posterior stabilized prosthesis. Results after follow-up of nine to twelve years. *J. Bone Joint Surg. Am.* 74:980-986.
6. Rodriguez JA, Bhende H, Ranawat CS. 2001. Total condylar knee replacement: a 20-year followup study. *Clin. Orthop. Relat Res.*388:10-17.
7. Catani F, Ensini A, Belvedere C, Feliciangeli A, Benedetti MG, Leardini A, Giannini S. 2009. In vivo kinematics and kinetics of a bi-cruciate substituting total knee arthroplasty: a combined fluoroscopic and gait analysis study. *J. Orthop. Res.* 27:1569-1575.
8. Catani F, Belvedere C, Ensini A, Feliciangeli A, Giannini S, Leardini A. 2011. In-vivo knee kinematics in rotationally unconstrained total knee arthroplasty. *J. Orthop. Res.* 29:1484-1490.

9. Abdel-Jaber S, Belvedere C, Leardini A, Affatato S. 2015. Wear simulation of total knee prostheses using load and kinematics waveforms from stair climbing. *J. Biomech.* 48(14):3830-3836.
10. Ranawat CS, Komistek RD, Rodriguez JA, Dennis DA, Anderle M. 2004. In vivo kinematics for fixed and mobile-bearing posterior stabilized knee prostheses. *Clin. Orthop. Relat Res.* 418:184-190.
11. Stiehl JB, Komistek RD, Dennis DA, Paxson RD, Hoff WA. 1995. Fluoroscopic analysis of kinematics after posterior-cruciate-retaining knee arthroplasty. *J. Bone Joint Surg. Br.* 77:884-889.
12. Mikulak SA, Mahoney OM, dela Rosa MA, Schmalzried TP. 2001. Loosening and osteolysis with the press-fit condylar posterior-cruciate-substituting total knee replacement. *J. Bone Joint Surg. Am.* 83-A:398-403.
13. Puloski SK, McCalden RW, MacDonald SJ, Rorabeck CH, Bourne RB. 2001. Tibial post wear in posterior stabilized total knee arthroplasty. An unrecognized source of polyethylene debris. *J. Bone Joint Surg. Am.* 83-A:390-397.
14. Mestha P, Shenava Y, D'Arcy JC. 2000. Fracture of the polyethylene tibial post in posterior stabilized (Insall Burstein II) total knee arthroplasty. *J. Arthroplasty* 15:814-815.
15. Callaghan JJ, O'Rourke MR, Goetz DD, Schmalzried TP, Campbell PA, Johnston RC. 2002. Tibial post impingement in posterior-stabilized total knee arthroplasty. *Clin. Orthop. Relat Res.* 404:83-88.
16. Silva M, Kabbash CA, Tiberi JV, III, Park SH, Reilly DT, Mahoney OM, Schmalzried TP. 2003. Surface damage on open box posterior-stabilized polyethylene tibial inserts. *Clin. Orthop. Relat Res.* 416:135-144.

17. Lombardi AV, Jr., Mallory TH, Fada RA, Adams JB, Kefauver CA. 2001. Fracture of the tibial spine of a Total Condylar III knee prosthesis secondary to malrotation of the femoral component. *Am. J. Knee Surg.* 14:55-59.
18. Banks SA, Markovich GD, Hodge WA. 1997. In vivo kinematics of cruciate-retaining and -substituting knee arthroplasties. *J. Arthroplasty* 12:297-304.
19. Bellemans J, Banks S, Victor J, Vandenneucker H, Moemans A. 2002. Fluoroscopic analysis of the kinematics of deep flexion in total knee arthroplasty. Influence of posterior condylar offset. *J. Bone Joint Surg. Br.* 84:50-53.
20. Dennis DA, Komistek RD, Mahfouz MR, Haas BD, Stiehl JB. 2003. Multicenter determination of in vivo kinematics after total knee arthroplasty. *Clin. Orthop. Relat Res.* 416:37-57.
21. Victor J, Mueller JK, Komistek RD, Sharma A, Nadaud MC, Bellemans J. 2010. In vivo kinematics after a cruciate-substituting TKA. *Clin. Orthop. Relat Res.* 468:807-814.
22. Sharma A, Komistek RD, Ranawat CS, Dennis DA, Mahfouz MR. 2007. In vivo contact pressures in total knee arthroplasty. *J. Arthroplasty* 22:404-416.
23. Cates HE, Komistek RD, Mahfouz MR, Schmidt MA, Anderle M. 2008. In vivo comparison of knee kinematics for subjects having either a posterior stabilized or cruciate retaining high-flexion total knee arthroplasty. *J. Arthroplasty* 23:1057-1067.
24. Nakamura S, Sharma A, Nakamura K, Ikeda N, Kawai J, Zingde SM, Komistek RD. 2015. In vivo kinematic effects of ball and socket third condyle as a post-cam mechanism in tri-condylar knee implants. *Knee* 22:237-242.
25. de Jong RJ, Heesterbeek PJ, Wymenga AB. 2010. A new measurement technique for the tibiofemoral contact point in normal knees and knees with TKR. *Knee Surg. Sports Traumatol. Arthrosc.* 18:388-393.

26. D'Lima DD, Poole C, Chadha H, Hermida JC, Mahar A, Colwell CW, Jr. 2001. Quadriceps moment arm and quadriceps forces after total knee arthroplasty. *Clin. Orthop. Relat Res.* 392:213-220.
27. Christen B, Heesterbeek P, Wymenga A, Wehrli U. 2007. Posterior cruciate ligament balancing in total knee replacement: the quantitative relationship between tightness of the flexion gap and tibial translation. *J. Bone Joint Surg. Br.* 89:1046-1050.
28. Heesterbeek PJ, Labey L, Wong P, Innocenti B, Wymenga AB. 2014. A new spacer-guided, PCL balancing technique for cruciate-retaining total knee replacement. *Knee Surg. Sports Traumatol. Arthrosc.* 22:650-659.
29. Wretenberg P, Ramsey DK, Nemeth G. 2002. Tibiofemoral contact points relative to flexion angle measured with MRI. *Clin. Biomech.* 17:477-485.
30. Dennis DA, Komistek RD, Mahfouz MR, Walker SA, Tucker A. 2004. A multicenter analysis of axial femorotibial rotation after total knee arthroplasty. *Clin. Orthop. Relat Res.* 428:180-189.
31. Victor J, Banks S, Bellemans J. 2005. Kinematics of posterior cruciate ligament-retaining and -substituting total knee arthroplasty: a prospective randomised outcome study. *J. Bone Joint Surg. Br.* 87:646-655.
32. Arnout N, Vanlommel L, Vanlommel J, Luyckx JP, Labey L, Innocenti B, Victor J, Bellemans J. 2014. Post-cam mechanics and tibiofemoral kinematics: a dynamic in vitro analysis of eight posterior-stabilized total knee designs. *Knee Surg. Sports Traumatol. Arthrosc.* 23(11):3343-3353.
33. Catani F, Innocenti B, Belvedere C, Labey L, Ensini A, Leardini A. 2010. The Mark Coventry Award: Articular contact estimation in TKA using in vivo kinematics and finite element analysis. *Clin. Orthop. Relat Res.* 468:19-28

34. Kurita M, Tomita T, Yamazaki T, Fujii M, Futai K, Shimizu N, Yoshikawa H, Sugamoto K. 2012. In vivo kinematics of high-flex mobile-bearing total knee arthroplasty, with a new post-cam design, in deep knee bending motion. *Int. Orthop.* 36:2465-2471.
35. Shimizu N, Tomita T, Yamazaki T, Yoshikawa H, Sugamoto K. 2014. In vivo movement of femoral flexion axis of a single-radius total knee arthroplasty. *J. Arthroplasty* 29:2407-2411.
36. Innocenti B, Pianigiani S, Labey L, Victor J, Bellemans J. 2011. Contact forces in several TKA designs during squatting: A numerical sensitivity analysis. *J. Biomech.* 44:1573-1581.
37. Pianigiani S, Chevalier Y, Labey L, Pascale V, Innocenti B. 2012. Tibio-femoral kinematics in different total knee arthroplasty designs during a loaded squat: a numerical sensitivity study. *J. Biomech.* 45:2315-2323.
38. Victor J, Bellemans J. 2006. Physiologic kinematics as a concept for better flexion in TKA. *Clin. Orthop. Relat Res.* 452:53-58.
39. Fantozzi S, Catani F, Ensini A, Leardini A, Giannini S. 2006. Femoral rollback of cruciate-retaining and posterior-stabilized total knee replacements: in vivo fluoroscopic analysis during activities of daily living. *J. Orthop. Res.* 24:2222-2229.
40. Belvedere C, Tamarri S, Notarangelo DP, Ensini A, Feliciangeli A, Leardini A. 2013. Three-dimensional motion analysis of the human knee joint: comparison between intra- and post-operative measurements. *Knee Surg. Sports Traumatol. Arthrosc.* 21:2375-2383.
41. van Duren BH, Pandit H, Price M, Tilley S, Gill HS, Murray DW, Thomas NP. 2012. Bicruciate substituting total knee replacement: how effective are the added kinematic constraints in vivo? *Knee Surg. Sports Traumatol. Arthrosc.* 20:2002-2010.

42. Ward TR, Burns AW, Gillespie MJ, Scarvell JM, Smith PN. 2011. Bicruciate-stabilised total knee replacements produce more normal sagittal plane kinematics than posterior-stabilised designs. *J. Bone Joint Surg. Br.* 93:907-913.
43. Insall JN, Dorr LD, Scott RD, Scott WN. 1989. Rationale of the Knee Society clinical rating system. *Clin. Orthop. Relat Res.* 248:13-14.
44. Banks SA, Hodge WA. 1996. Accurate measurement of three-dimensional knee replacement kinematics using single-plane fluoroscopy. *IEEE Trans. Biomed. Eng* 43:638-649.
45. Grood ES, Suntay WJ. 1983. A joint coordinate system for the clinical description of three-dimensional motions: application to the knee. *J. Biomech. Eng* 105:136-144.
46. Godest AC, Beaugin M, Haug E, Taylor M, Gregson PJ. 2002. Simulation of a knee joint replacement during a gait cycle using explicit finite element analysis. *J. Biomech.* 35:267-275.
47. Halloran JP, Petrella AJ, Rullkoetter PJ. 2005. Explicit finite element modeling of total knee replacement mechanics. *J. Biomech.* 38:323-331.
48. Komistek RD, Dennis DA, Mahfouz M. 2003. In vivo fluoroscopic analysis of the normal human knee. *Clin. Orthop. Relat Res.* 410:69-81.
49. Moro-oka TA, Hamai S, Miura H, Shimoto T, Higaki H, Fregly BJ, Iwamoto Y, Banks SA. 2008. Dynamic activity dependence of in vivo normal knee kinematics. *J. Orthop. Res.* 26:428-434.
50. Meccia B, Komistek RD, Mahfouz M, Dennis D. 2014. Abnormal axial rotations in TKA contribute to reduced weightbearing flexion. *Clin. Orthop. Relat Res.* 472:248-253.

FIGURE CAPTIONS

Figure 1: Average antero-posterior displacement of the lateral (left) and medial (right) contact points on corresponding tibial condyles plotted versus knee flexion. Standard deviation is also reported at each 10° flexion. The three motor tasks are shown separately, chair rising (A), stair climbing (B), and step-up (C).

Figure 2: Average tibio-femoral axial rotation plotted versus knee flexion for the three motor tasks. Negative and positive values correspond to external and internal rotation, respectively. Standard deviation is also reported at each 10° flexion.

Figure 3: Position of the pivot points in chair rising for each patient (blue dots) and on average over patients (red dot). These are plotted in % locations over the antero-posterior length of the tibial insert, -50% and 50% being the most posterior and most anterior location, respectively, and over the medio-lateral width of the tibial insert, -50% and 50% being the most lateral and most medial location, respectively.

Figure 4: Position of the pivot points in stair climbing (same graphical representation as in Figure 3).

Figure 5: Position of the pivot points in step-up (same graphical representation as in Figure 3).

Figure 6: Position of the pivot points (same graphical representation as in Figure 3) in all the three motor tasks analyzed for each patient (blue dots) and on average among all tasks and patients (red dot).

Figure 7: Percentage of patients where the post-cam contact occurred at a certain knee flexion angle reported for the three motor tasks. Anterior (A) and posterior (B) parts of the post-cam are shown separately.

Table 1: Patients' demographic data.

Patient	Age (Years)	Body Mass Index	Gender (M=male; F= female)	Side (L=left; R=right)
1	58	36	<i>F</i>	<i>R</i>
2	69	25	<i>M</i>	<i>R</i>
3	69	33	<i>F</i>	<i>R</i>
4	68	26	<i>M</i>	<i>L</i>
5	77	23	<i>F</i>	<i>R</i>
6	65	29	<i>F</i>	<i>R</i>
7	69	31	<i>F</i>	<i>R</i>
8	75	24	<i>F</i>	<i>L</i>
9	69	34	<i>F</i>	<i>R</i>
10	71	28	<i>M</i>	<i>R</i>
11	75	25	<i>M</i>	<i>R</i>
12	75	21	<i>F</i>	<i>L</i>
13	75	24	<i>F</i>	<i>R</i>
14	72	30	<i>M</i>	<i>L</i>
15	80	31	<i>F</i>	<i>R</i>
Average	71.1±5.4	28.0±4.4	---	---

Table2: Amplitude of contact line rotation and location of the pivot point reported for each patient and for each motor task throughout knee flexion range. The latter is reported in % locations over the antero-posterior (AP) length of the tibial insert, -50% and 50% being the most posterior and most anterior location respectively, and over the medio-lateral (ML) width of the tibial insert, -50% and 50% being the most lateral and most medial location respectively.

Patient	Amplitude of Contact Line Rotation (°)			Pivot Point ML Location (%)			Pivot Point AP Location (%)		
	<i>Chair Rising-Sitting</i>	<i>Stair Climbing</i>	<i>Step Up-Down</i>	<i>Chair Rising-Sitting</i>	<i>Stair Climbing</i>	<i>Step Up-Down</i>	<i>Chair Rising-Sitting</i>	<i>Stair Climbing</i>	<i>Step Up-Down</i>
1	13.4	11.6	9.1	79	89	6	-1	-11	-8
2	20.1	5.6	10.3	28	30	40	-6	-11	-11
3	16.7	19.1	22.7	38	40	56	-2	-2	-4
4	15.2	8.7	15.8	51	24	35	-15	-14	-16
5	18.0	2.4	10.9	51	164	36	-19	-1	-12
6	14.4	12.2	13.8	4	131	21	-5	-1	-6
7	17.1	2.6	11.5	14	25	34	-13	-4	-6
8	7.8	16.4	10.3	109	57	42	-4	-13	-24
9	6.9	19.5	11.4	5	10	16	-9	-13	-10
10	8.7	6.6	35.7	53	18	33	-28	-9	-27
11	18.6	14.0	12.8	14	8	7	-11	-13	-9
12	19.3	4.2	9.8	53	6	63	-18	-17	-21
13	13.4	14.6	4.6	84	19	44	-5	-7	-11
14	9.8	9.4	10.2	18	8	51	-14	-7	0
15	7.7	2.2	3.9	6	57	19	-14	-1	-12
Average	13.8±4.6	9.9±6.0	12.9±7.7	40.5±32.1	45.7±47.6	33.5±17.0	-10.9±7.4	-8.3±5.4	-11.8±7.4

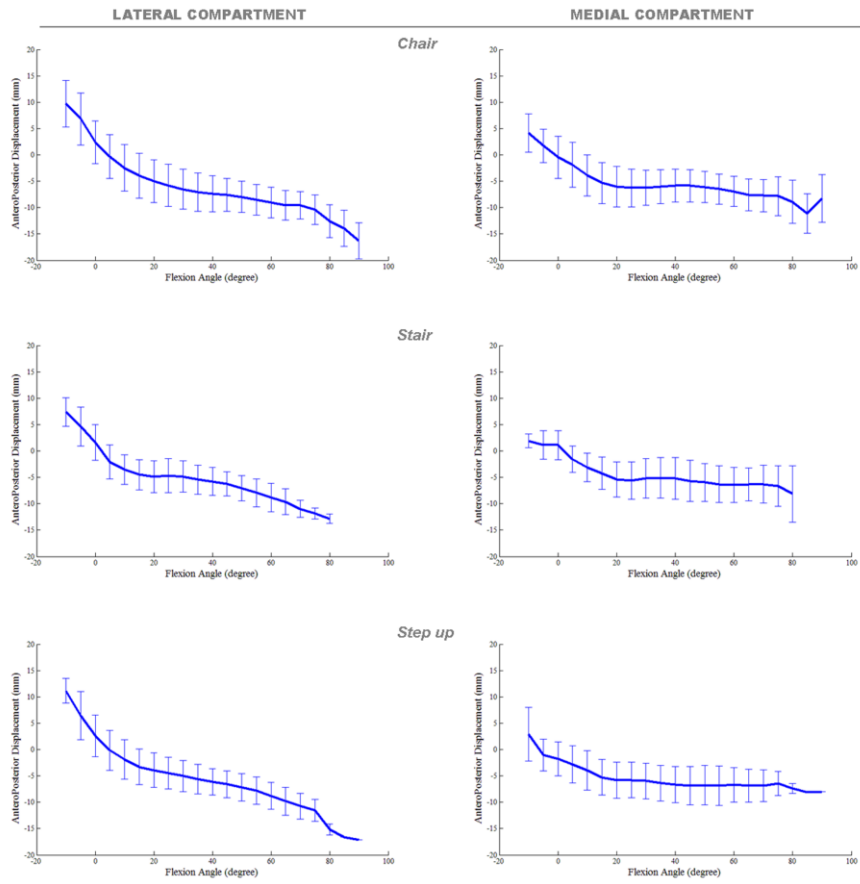


Figure 1

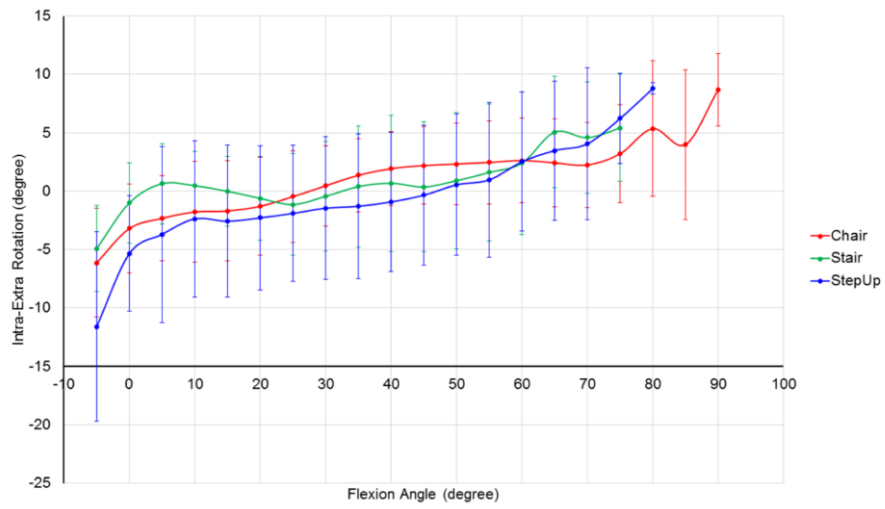


Figure 2

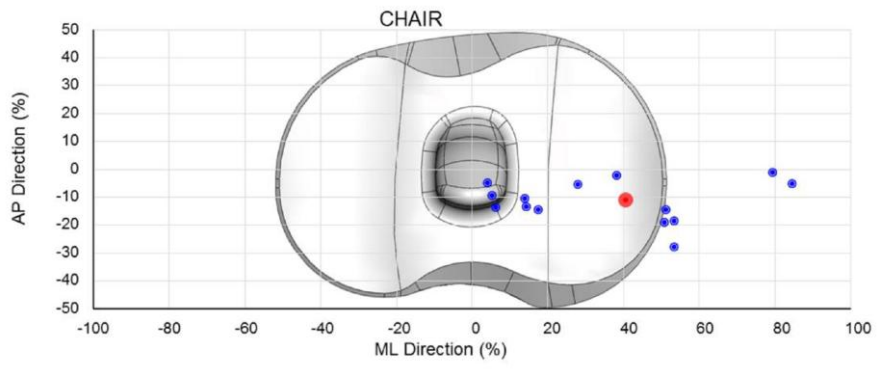


Figure 3

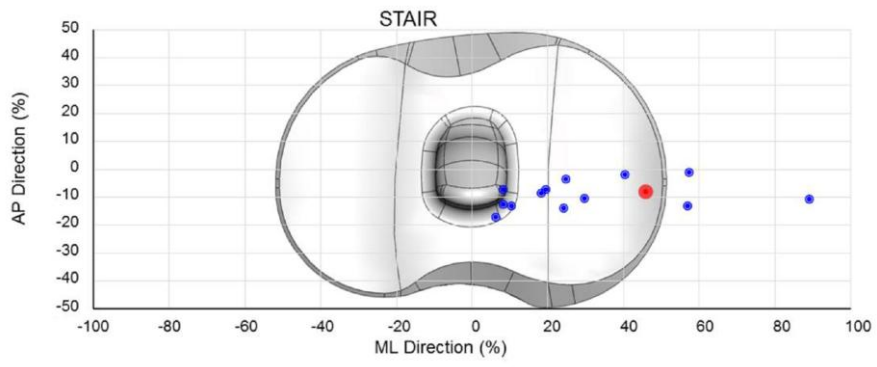


Figure 4

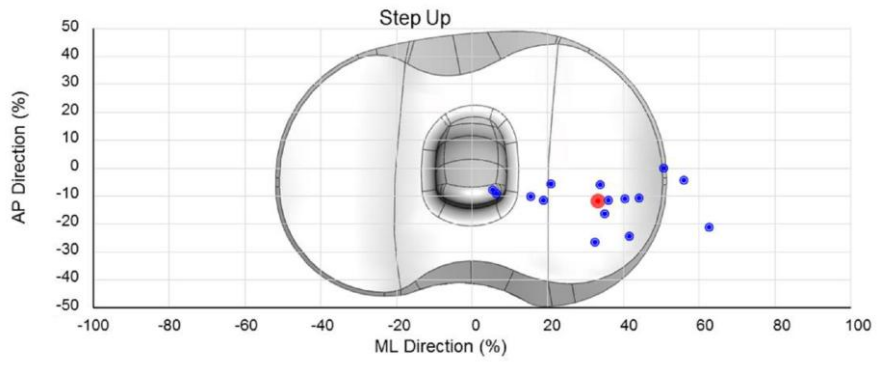


Figure 5

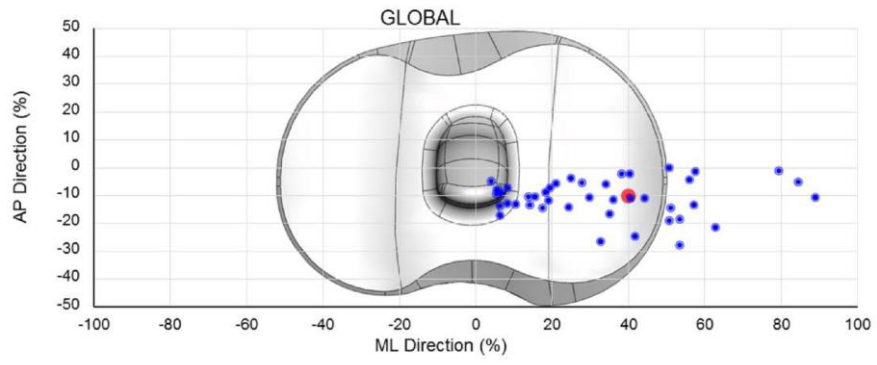


Figure 6

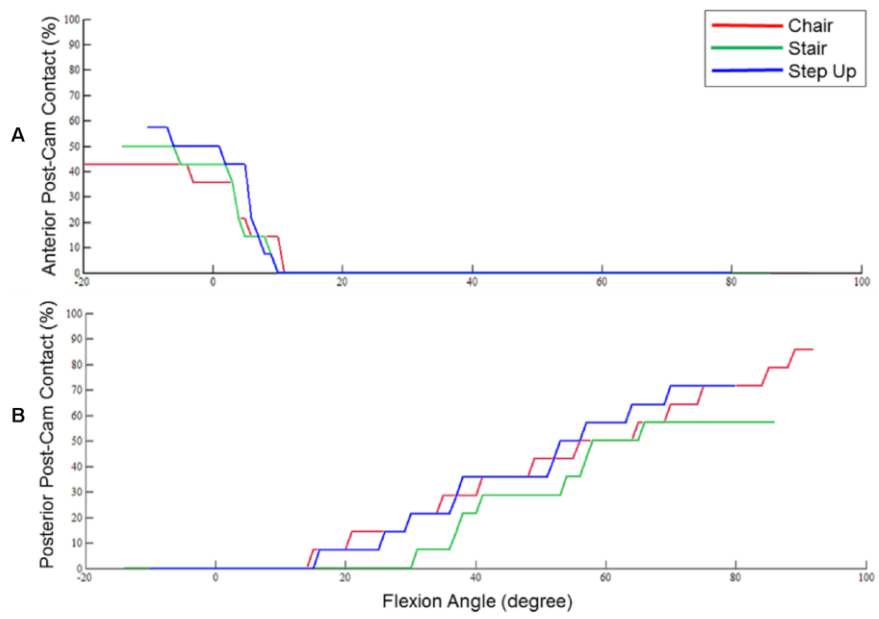


Figure 7